



Deluxe Bedside Assist Wave Handle (w/out legs)

300 LBS
WEIGHT CAPACITY

H5001





Prior to use, please read all instructions and inspect all parts carefully for damage prior to assembly.

H5001

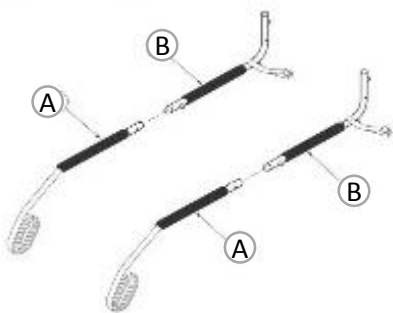
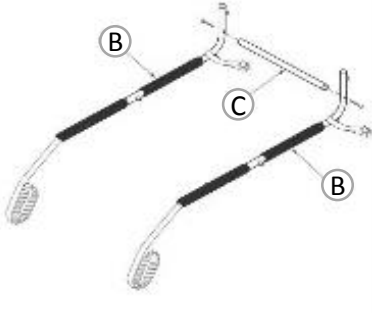
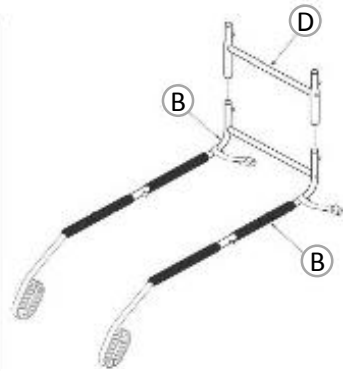
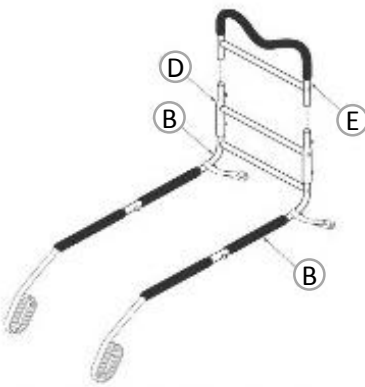
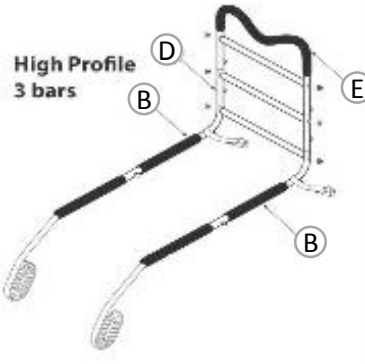
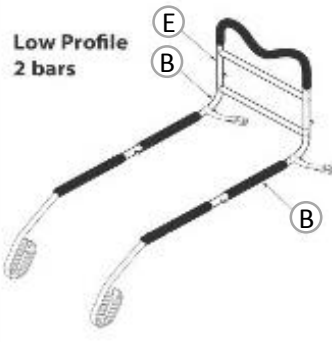
Cautions and warnings

1. Please read these instructions carefully before installing and using the bed rail.
2. This bar is not designed to support the entire weight of a person and is only suitable for people weighing less than 135 kg.
3. Narrow beds can be tilted if user puts full body weight on the handle.
4. The adjustable bed bar is not intended for people with reduced mobility or people who are permanently bedridden. Additional safety measures and precautions should be used in high-risk patients.
5. The bed rail must not be attached to a medical bed that can move or be lifted.
6. The mattress must be tight against the grab bar without leaving any space to prevent a person from getting trapped. This should be checked frequently, if not daily.
7. For added safety, we recommend that you install two bed rails, one on each side of the bed, to help hold the mattress in place, without leaving any space.

Warning: If the box spring is wider than the mattress, two bed rails will not work.

Assembly Instructions


1. Remove all parts from carton and dispose of plastic wrapping safely keeping away from children and infants.
2. The handle has 2 settings. For Low Profile, use (2) crossbars or use three (3) crossbars for High Profile.
(For thick mattresses, using 3 crossbars is recommended. At the Low Profile setting, part D is not required and should be saved for possible future use.)

Assembling the		
 3. Insert part A into part B on each side.	 4. Connect part C into parts B on each side using provided allen key. Do not tighten.	 5. For High Profile, connect part D (H-bar), to part B. Skip this step for Low Profile and store part D.
 6. Lastly, insert part E making sure that all spring buttons are in place. Tighten all screws snugly.	 High Profile 3 bars	 Low Profile 2 bars
*Tip : If connecting part D to part E is difficult, slightly loosen the screws connecting part C. Re-insert part E into part D making sure the spring buttons are in place and re-tighten screws.		


Installation Instructions

1. For easier installation, remove the mattress and place the assembled Rail on top of the boxspring.

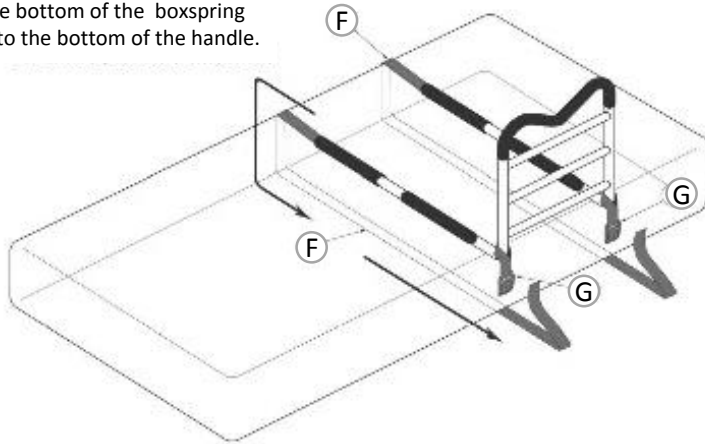2. Run the long webbing (part F) around the bottom of the boxspring and back to the bottom of the handle.




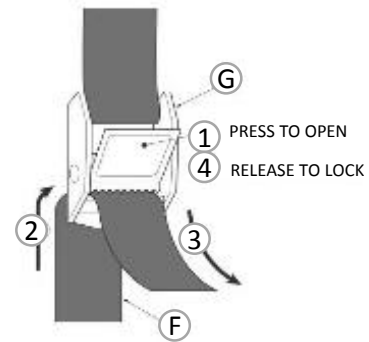3. Feed the webbing through the buckle (part G) and lock the buckle to secure the strap at the desired length. Repeat on other side.




4. If removed, replace the mattress.
5. Lie on the bed and move the bed rail to the desired position
6. Making sure the webbing straps are straight and parallel, tighten them securely against the boxspring.
7. Loop and tuck the loose end of the webbing directly below the buckle to prevent tripping hazards.

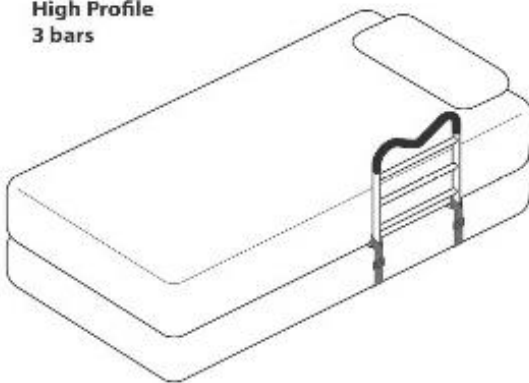**High Profile
3 bars**



**Low Profile
2 bars**

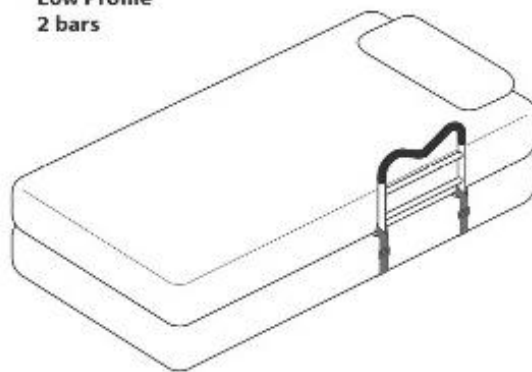

IMPORTANT : For your safety, Part F Safety Strap set provided with this bedrail **MUST** be installed as shown above



Lifestyle Mobility Aids
3200 Tyrone Blvd. N.
St. Petersburg, FL

EC REP



Care and Maintenance

Clean frame with soap and water, dry with towel.

Check straps and handles periodically to make sure they are not torn, worn or missing. Replace if necessary.

Persons with severe disabilities or persons who are unable to walk without an aide should not attempt to use this product without assistance.

Maximum user weight : 300 lbs



LIFESTYLE MOBILITY AIDS
3200 Tyrone Blvd N
St. Petersburg, FL 33710

Email: contactus@lifestylemobilityaids.com
Website: www.lifestylemobilityaids.com

v:1 2/26/21